

Pressure Injectable Jugular Axillo-Subclavian Central Catheter (JACC) Product

Rx only.

Indications:

The Arrow® Pressure Injectable JACC with Arrowg+ard Blue Advance™ Antimicrobial and Antithrombogenic Protection is indicated for short-term (< 30 days) or long-term (> 30 days) access to the central venous system for intravenous therapy, blood sampling, infusion, pressure injection of contrast media and allows for central venous pressure monitoring. The maximum pressure of pressure injector equipment used with the Pressure Injectable JACC may not exceed 300 psi (2068.4 kPa). The maximum pressure injection flow rate for the specific lumen being used for pressure injection is printed on the extension line hub.

Contraindications:

None known. See additional labeling for product specific contraindications.

General Warnings and Cautions

Warnings:

1. Sterile, Single use: Do not reuse, reprocess or resterilize. Reuse of device creates a potential risk of serious injury and/or infection which may lead to death.
2. Read all package insert warnings, precautions and instructions prior to use. Failure to do so may result in severe patient injury or death.
3. Do not place catheter into or allow it to remain in the right atrium or right ventricle to reduce risk of patient injury. X-ray exam or other method must show catheter tip located in lower 1/3 of the Superior Vena Cava (SVC), in accordance with institutional policies and procedures.
4. Clinicians must be aware of potential entrapment of the guidewire by any implanted device in circulatory system. It is recommended that if patient has a circulatory system implant, catheter procedure be done under direct visualization to reduce risk of guidewire entrapment.
5. Do not use excessive force when introducing guidewire, peel-away sheath over tissue dilator, or tissue dilator as this can lead to vessel perforation, bleeding, or component damage.
6. Passage of guidewire into the right heart can cause dysrhythmias and a perforation of vessel, atrial or ventricular wall.
7. Do not apply excessive force in placing or removing catheter or guidewire. Excessive force can cause component damage or breakage. If damage is suspected or withdrawal cannot be easily accomplished, radiographic visualization should be obtained and further consultation requested.
8. Use only lumen(s) labeled "Pressure Injectable" for pressure injection to reduce risk of catheter failure and/or patient complications. Refer to the Pressure Injectable ARROW® JACC Information card for pressure injection instructions and information.
9. Do not secure, staple and/or suture directly to outside diameter of catheter body or extension lines to reduce risk of cutting or damaging the catheter or impeding catheter flow. Secure only at indicated stabilization locations.

10. Clinicians should be aware that slide clamps may be inadvertently removed. Air embolism can occur if air is allowed to enter a central venous access device or vein. Do not leave open needles, sheaths, or uncapped, unclamped catheters in central venous puncture site. Use only securely tightened Luer-Lock connections with any central venous access device to guard against inadvertent disconnection.

11. Clinicians must be aware of complications associated with central venous catheters including, but not limited to:

- cardiac tamponade secondary to vessel, atrial, or ventricular perforation
- pleural (i.e., pneumothorax) and mediastinal injuries
- air embolism
- catheter embolism
- catheter occlusion
- thoracic duct laceration
- bacteremia
- septicemia
- thromboembolism
- thrombosis
- inadvertent arterial puncture
- nerve injury/damage
- hematoma
- hemorrhage
- fibrin sheath formation
- exit site infection
- vessel erosion
- catheter tip malposition
- dysrhythmias
- brachial plexus injury
- phlebitis
- anaphylaxis

Cautions:

1. Do not alter the catheter except as instructed. Do not alter the guidewire or any other kit/set component during insertion, use or removal.
2. Procedure must be performed by trained personnel well versed in anatomical landmarks, safe technique and potential complications.
3. Use standard precautions and follow established institutional policies and procedures.
4. Some disinfectants used at catheter insertion site contain solvents which can weaken the catheter material. Alcohol, acetone, and polyethylene glycol can weaken the structure of polyurethane materials. These agents may also weaken the adhesive bond between catheter stabilization device and skin.
 - Do not use acetone on catheter surface.
 - Do not use alcohol to soak catheter surface or allow alcohol to dwell in a catheter lumen to restore catheter patency or as an infection prevention measure.
 - Do not use polyethylene glycol containing ointments at insertion site.
 - Take care when infusing drugs with a high concentration of alcohol.
 - Allow insertion site to dry completely prior to applying dressing.

5. Ensure catheter patency prior to use, including prior to pressure injection. Do not use syringes smaller than 10 mL (a fluid filled 1 mL syringe can exceed 300 psi [2068.4 kPa]) to reduce risk of intraluminal leakage or catheter rupture. Power injector equipment may not prevent overpressurizing an occluded or partially occluded catheter.
6. Minimize catheter manipulation throughout procedure to maintain proper catheter tip position.

Kits/Sets may not contain all accessory components detailed in these instructions for use. Become familiar with instructions for individual component(s) before beginning the procedure.

A Suggested Procedure: Use sterile technique.

Prep Puncture Site:

1. Position patient as appropriate for insertion site.
 - Axillary, Subclavian or Jugular approach: Place patient in slight Trendelenburg position as tolerated to reduce risk of air embolism and enhance venous filling.
2. Prepare clean skin with an appropriate antiseptic agent.
3. Drape puncture site.
4. Administer local anesthetic per institutional policies and procedures.

SharpsAway II™ Locking Disposal Cup (where provided):

The SharpsAway II™ Locking Disposal Cup is used for disposal of needles (15 Ga. - 30 Ga.).

- Using one-handed technique, firmly push needles into disposal cup holes (refer to Figure 1).




Figure 1

- Once placed into disposal cup, needles will be automatically secured in place so that they cannot be reused.

⚠ Caution: Do not attempt to remove needles that have been placed into SharpsAway II Locking Disposal Cup. These needles are secured in place. Damage may occur to needles if they are forced out of disposal cup.

- Where provided, a foam SharpsAway® system may be utilized by pushing needles into foam after use.

⚠ Caution: Do not re-use needles after they have been placed into the foam SharpsAway system. Particulate matter may adhere to needle tip.

Prepare Catheter: Trim Catheter if Required

Note: Trimming catheter may lead to precipitation from the infusion of incompatible drugs since the exit ports may no longer be staggered.

5. Retract contamination guard.
6. The catheter is marked to identify desired amount of catheter to be trimmed and length of catheter that remains (refer to Figure 2).




Figure 2

NOTE: Centimeter double numbering pattern is as follows (refer to Figure 2):

- First number designates centimeters from tip of catheter
- Second number designates centimeters from hub of catheter

7. Cut catheter straight across (90° to catheter cross-section) using trimming device (where provided) to maintain a blunt tip.

⚠ Caution: Do not cut the catheter when a wire or stylet is in the catheter to reduce risk of damage or embolism.

Catheter Trimmer (where provided):

A catheter trimmer is a one-time use trimming device. Insert catheter into hole on trimmer to desired cut location. Depress blade to cut catheter.

8. Inspect cut surface for clean cut and no loose material.
9. Flush each lumen with sterile normal saline for injection to establish patency and prime lumen(s).
10. Clamp or attach Luer-Lock connector(s) to extension line(s) to contain saline within lumen(s).

Gain Initial Venous Access:

Echogenic Needle (where provided):

An echogenic needle is used to allow access to the vascular system for the introduction of a guidewire to facilitate catheter placement. The needle tip is enhanced for approximately 1 cm for clinician to identify exact needle tip location when puncturing the vessel under ultrasound.

Protected Needle/Safety Needle (where provided):

A protected needle/safety needle should be used in accordance with manufacturer's instructions for use.

11. Insert introducer needle or catheter/needle with attached syringe into vein and aspirate.

⚠ Warning: Do not leave open needles or uncapped, unclamped catheters in central venous puncture site. Air embolus can occur with these practices.

⚠ Caution: Do not reinsert needle into introducer catheter (where provided) to reduce risk of catheter embolus.

Verify Venous Access:

Utilize one of the following techniques to verify venous access because of the potential for inadvertent arterial placement:

- Central Venous Waveform
- Pulsatile Flow (if hemodynamic monitoring equipment is not available):
 - Disconnect syringe from needle and observe for pulsatile flow.

⚠ Warning: Pulsatile flow is usually an indicator of inadvertent arterial puncture.

⚠ Caution: Do not rely on blood aspirate color to indicate venous access.

Insert Guidewire:

Guidewire:

Kits/Sets are available with a variety of guidewires. Guidewires are provided in different diameters, lengths and tip configurations for specific insertion techniques. Become familiar with the guidewire(s) to be used with the specific technique before beginning the actual insertion procedure.

Prepare guidewire for insertion by wetting guidewire with sterile normal saline for injection. Ensure that guidewire remains lubricious until it is inserted into patient.

⚠ Warning: Do not insert stiff end of guidewire into vessel as this may result in vessel damage.

Arrow Advancer (where provided):

Arrow Advancer is used to introduce guidewire into a needle.

- Using thumb, retract guidewire tip. Place tip of Arrow Advancer – with guidewire retracted – into introducer needle (refer to Figure 3).




Figure 3

12. Advance guidewire into introducer needle.

- Raise thumb and pull Arrow Advancer approximately 4 - 8 cm away from introducer needle. Lower thumb onto Arrow Advancer and while maintaining a firm grip on guidewire, push assembly into needle to further advance guidewire. Continue until guidewire reaches desired depth.

- Use centimeter markings (where provided) on guidewire as a reference to assist in determining how much guidewire has been inserted.

⚠ Caution: Maintain firm grip on guidewire at all times. Keep sufficient guidewire length exposed for handling purposes. A non-controlled guidewire can lead to wire embolus.

⚠ Warning: Do not withdraw guidewire against needle bevel to reduce risk of possible severing or damaging of guidewire.

- Remove introducer needle (or catheter) while holding guidewire in place.
- If necessary, enlarge cutaneous puncture site with cutting edge of scalpel, positioned away from guidewire.

⚠ Warning: Do not cut guidewire to alter length.

⚠ Warning: Do not cut guidewire with scalpel.

- Position cutting edge of scalpel away from guidewire.
- Engage safety and/or locking feature of scalpel (where provided) when not in use to reduce the risk of sharps injury.

- Use tissue dilator to enlarge tissue tract to the vein as required (where provided). Follow the angle of the guidewire slowly through the skin.

⚠ Warning: Do not leave tissue dilator in place as an indwelling catheter. Leaving tissue dilator in place puts patient at risk for possible vessel wall perforation.

Place Peel-Away Sheath for Modified Seldinger Insertion:

- Thread peel-away sheath/dilator assembly over guidewire.
- Grasping near skin, advance sheath/dilator assembly with slight twisting motion to a depth sufficient to enter vessel.

Note: A slight twisting motion may help sheath advancement.

⚠ Caution: Sufficient guidewire length must remain exposed at hub end of sheath to maintain a firm grip on guidewire.

- Check sheath placement by holding sheath in place, twisting dilator hub counterclockwise to release dilator hub from sheath hub, withdraw guidewire and dilator sufficiently to allow blood flow.

- Holding sheath in place, remove guidewire and dilator as a unit.

⚠ Warning: Do not apply undue force on guidewire to reduce risk of possible breakage.

⚠ Warning: Do not leave tissue dilator in place as an indwelling catheter. Leaving tissue dilator in place puts patient at risk for possible vessel wall perforation.

- Quickly place finger or thumb over sheath end upon removal of dilator and guidewire to reduce risk of air entry.

- Always verify entire guidewire is intact upon removal.

Advance Catheter:

- Retract contamination guard.

Catheter Insertion with Modified Seldinger Technique:

- Insert catheter through peel-away sheath to final indwelling position.
- Withdraw peel-away sheath over catheter until free from venipuncture site.
- Grasp tabs of peel-away sheath and pull apart, away from catheter while withdrawing from vessel (refer to Figure 4) until sheath splits down its entire length.

⚠ Caution: Avoid tearing sheath at insertion site which opens surrounding tissue creating a gap between the catheter and dermis.

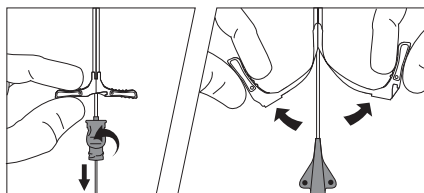


Figure 4

Catheter Insertion with Seldinger Technique:

- Uncap distal extension line for guidewire passage.
- Use centimeter markings (where provided) on guidewire to adjust indwelling length to desired depth of indwelling catheter placement.
- Thread tip of catheter over guidewire. Sufficient guidewire length must remain exposed at hub of catheter to maintain a firm grip on guidewire.
- Grasping near skin, advance catheter into vein with a slight twisting motion.

⚠ Warning: Do not attach catheter clamp and fastener (where provided) until guidewire is removed.

- Hold catheter at desired depth and remove guidewire. Always verify entire guidewire is intact upon removal.

⚠ Warning: Do not apply undue force on guidewire to reduce risk of possible breakage.

- Using centimeter marks on catheter as positioning reference points, advance catheter to final indwelling position.

Complete Catheter Insertion:

- Check lumen patency by attaching a syringe to each extension line and aspirate until free flow of venous blood is observed.
- Flush lumen(s) to completely clear blood from catheter.
- Connect all extension line(s) to appropriate Luer-Lock connector(s) as required. Unused port(s) may be "locked" through Luer-Lock connector(s) using standard institutional policies and procedures.
 - Slide clamp(s) are provided on extension lines to occlude flow through each lumen during line and Luer-Lock connector changes.

⚠ Warning: Open slide clamp prior to infusion through lumen to reduce risk of damage to extension line from excessive pressure.

Secure Catheter:

- Use a catheter stabilization device, catheter clamp and fastener, staples or sutures (where provided).
 - Use triangular juncture hub with side wings as primary suture site.
 - Use catheter clamp and fastener as a secondary suture site as necessary.

⚠ Caution: Minimize catheter manipulation throughout procedure to maintain proper catheter tip position.

Catheter Stabilization Device (where provided):

A catheter stabilization device should be used in accordance with manufacturer's instructions for use.

Catheter Clamp and Fastener (where provided):

A catheter clamp and fastener are used to secure catheter when an additional securement site other than the catheter hub is required for catheter stabilization.

⚠ Warning: Do not attach catheter clamp and fastener (where provided) until guidewire is removed.

- After guidewire has been removed and necessary lines have been connected or locked, spread wings of rubber clamp and position on catheter making sure catheter is not moist, as required, to maintain proper tip location.
- Snap rigid fastener onto catheter clamp.
- Secure catheter clamp and fastener as a unit to patient by using either catheter stabilization device, stapling or suturing. Both catheter clamp and fastener need to be secured to reduce risk of catheter migration (refer to Figure 5).




Figure 5

30. Ensure insertion site is dry before applying dressing per manufacturer's instructions.
31. Assess catheter tip placement in compliance with institutional policies and procedures.
32. If catheter tip is malpositioned, assess the situation and replace the catheter or reposition according to institutional policies and procedures.

Care and Maintenance:

Dressing:

Dress according to institutional policies, procedures, and practice guidelines. Change immediately if the integrity becomes compromised (e.g. dressing becomes damp, soiled, loosened or no longer occlusive).

Catheter Patency:

Maintain catheter patency according to institutional policies, procedures and practice guidelines. All personnel who care for patients with central venous catheters must be knowledgeable about effective management to prolong catheter's dwell time and prevent injury.

Catheter Removal Instructions:

1. Position patient as clinically indicated to reduce risk of potential air embolus.
2. Remove dressing.
3. Release catheter and remove from catheter securement device(s).
4. Ask patient to take a breath and hold it if removing internal jugular or subclavian catheter.
5. Remove catheter by slowly pulling it parallel to skin. If resistance is met while removing catheter **STOP**

⚠ Caution: Catheter should not be forcibly removed, doing so may result in catheter breakage and embolization. Follow institutional policies and procedures for difficult to remove catheter.

6. Apply direct pressure to site until hemostasis is achieved followed by an ointment-based occlusive dressing.

⚠ Warning: Residual catheter track remains an air entry point until site is epithelialized. Occlusive dressing should remain in place for at least 24 hours or until site appears epithelialized.

7. Document catheter removal procedure including confirmation that entire catheter length and tip has been removed per institutional policies and procedures.

For reference literature concerning patient assessment, clinician education, insertion technique, and potential complications associated with this procedure, consult standard textbooks, medical literature, and Arrow International, Inc. website: www.teleflex.com

en Symbol Glossary								
Caution	Consult instructions for use	Do not reuse	Do not resterilize	Sterilized by ethylene oxide	Keep away from sunlight	Keep dry	Do not use if package is damaged	Not made with natural rubber latex
Catalogue number	Lot number	Use by	Manufacturer					

Teleflex, the Teleflex logo, Arrow, the Arrow logo, SharpsAway and SharpsAway II are trademarks or registered trademarks of Teleflex Incorporated or its affiliates, in the U.S. and/or other countries. © 2015 Teleflex Incorporated. All rights reserved.