

Tegaderm™

Transparent Dressing Instructions

1. Prepare site. Allow all preps to dry completely.
2. Remove liner to expose adhesive (refer to Fig. 1).

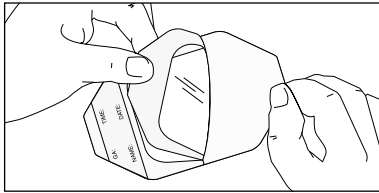


Fig. 1

3. Place without tension over site. Smooth down dressing edges while removing the frame (refer to Fig. 2).

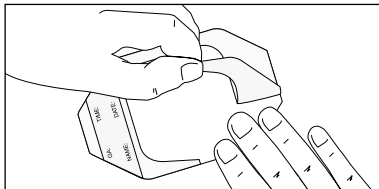


Fig. 2

4. Record dressing change information and apply label near site (refer to Fig. 3).

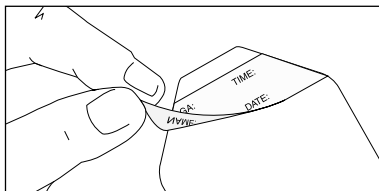


Fig. 3

M-05500-102A (1/01)

Tegaderm™

Transparent Dressing Instructions

1. Prepare site. Allow all preps to dry completely.
2. Remove liner to expose adhesive (refer to Fig. 1).

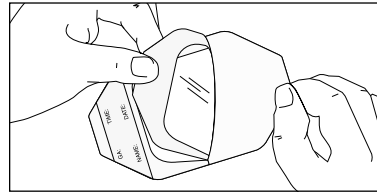


Fig. 1

3. Place without tension over site. Smooth down dressing edges while removing the frame (refer to Fig. 2).

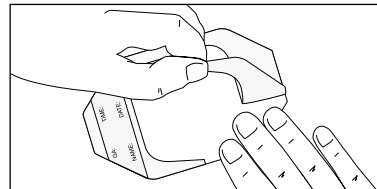


Fig. 2

4. Record dressing change information and apply label near site (refer to Fig. 3).

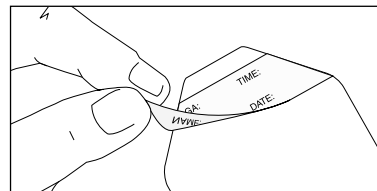


Fig. 3

M-05500-102A (1/01)

Tegaderm™

Transparent Dressing Instructions

1. Prepare site. Allow all preps to dry completely.
2. Remove liner to expose adhesive (refer to Fig. 1).

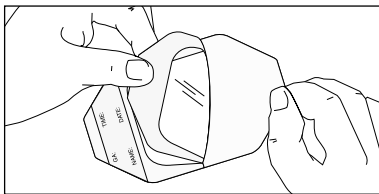


Fig. 1

3. Place without tension over site. Smooth down dressing edges while removing the frame (refer to Fig. 2).

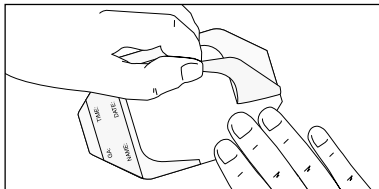


Fig. 2

4. Record dressing change information and apply label near site (refer to Fig. 3).

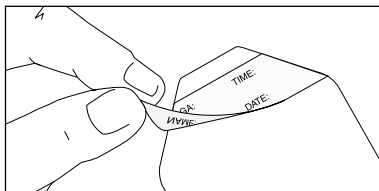


Fig. 3

M-05500-102A (1/01)

Tegaderm™

Transparent Dressing Instructions

1. Prepare site. Allow all preps to dry completely.
2. Remove liner to expose adhesive (refer to Fig. 1).

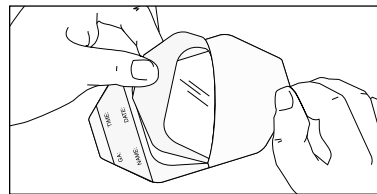


Fig. 1

3. Place without tension over site. Smooth down dressing edges while removing the frame (refer to Fig. 2).

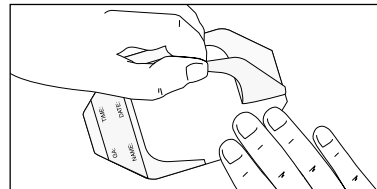


Fig. 2

4. Record dressing change information and apply label near site (refer to Fig. 3).

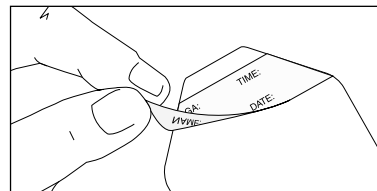


Fig. 3

M-05500-102A (1/01)